




Hook-and-Loop Seatbelt

Instructions for Use, Application, and Care

Use

Hook-and-Loop Seatbelts are used with an alarm to indicate to staff when a patient is attempting to get out of a wheelchair. The yellow loop handle is easy to release with a simple sweeping motion that does not require individual finger dexterity. Hook-and-Loop Seatbelts are not intended to be used as a restraint. Three seatbelt attachment options: Bolting, UniLoop fastener, and Zip Ties.

Application

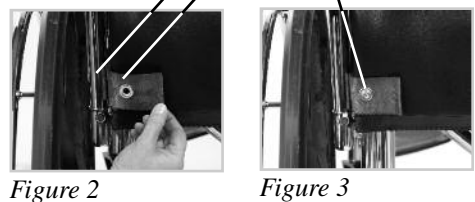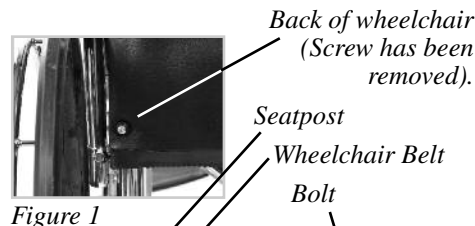



Setup Options

Bolting seatbelt directly to the wheelchair

1. Remove the lower screw on both sides of the back of the chair. *Figure 1*
2. Pass the belt between the seat posts and arm rests. *Figure 2*
3. Reinsert the screw through the grommet to attach belt to wheelchair. *Figure 3*


Attaching seatbelt with UniLoop

1. Begin by attaching carabiner clip to the grommet located at each end of the seatbelt. *Figure 4*
2. Wrap UniLoop around the wheelchair back's upright tubing on both sides of the wheelchair. *Figure 5*



Attaching the seatbelt with Zip Ties

1. Insert the Zip Ties through the grommets on the belt. *Figure 6*
2. Wrap the Zip Ties around the chair posts. *Figure 7*
3. Tighten around chair posts.



Manufactured for:



MDSS GmbH
Schiffgraben 41
D-30175 Hannover,
Germany



AliMed® inc.

297 High Street
Dedham, MA 02026-9135 U.S.A.
PH 800-225-2610 • FAX 800-437-2966

AliMed.com

#6583REV0315 CCO746

©2015 AliMed® inc. All rights reserved.

Made in Taiwan




Hook-and-Loop Seatbelt

Instructions for Use, Application, and Care

Use

Hook-and-Loop Seatbelts are used with an alarm to indicate to staff when a patient is attempting to get out of a wheelchair. The yellow loop handle is easy to release with a simple sweeping motion that does not require individual finger dexterity. Hook-and-Loop Seatbelts are not intended to be used as a restraint. Three seatbelt attachment options: Bolting, UniLoop fastener, and Zip Ties.

Application

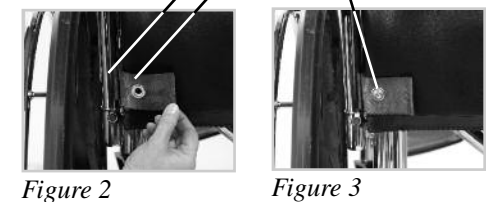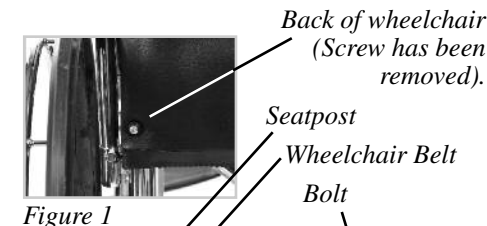



Setup Options

Bolting seatbelt directly to the wheelchair

1. Remove the lower screw on both sides of the back of the chair. *Figure 1*
2. Pass the belt between the seat posts and arm rests. *Figure 2*
3. Reinsert the screw through the grommet to attach belt to wheelchair. *Figure 3*


Attaching seatbelt with UniLoop

1. Begin by attaching carabiner clip to the grommet located at each end of the seatbelt. *Figure 4*
2. Wrap UniLoop around the wheelchair back's upright tubing on both sides of the wheelchair. *Figure 5*



Attaching the seatbelt with Zip Ties

1. Insert the Zip Ties through the grommets on the belt. *Figure 6*
2. Wrap the Zip Ties around the chair posts. *Figure 7*
3. Tighten around chair posts.



Manufactured for:



MDSS GmbH
Schiffgraben 41
D-30175 Hannover,
Germany



AliMed® inc.

297 High Street U.S.A.
PH 800-225-2610 • FAX 800-437-2966

AliMed.com

#6583REV0315 CCO746

©2015 AliMed® inc. All rights reserved.

Made in Taiwan

Seatbelt Adjustment and Fit

Secure seatbelt around the patient, *Figures 8 and 9*. Adjust seatbelt length by sliding buckle to shorten or increase length, *Figures 10 and 11*. If additional length is needed, a seatbelt extender (#79205) may be purchased separately.

Plug cord from seatbelt into alarm, *Figure 12*. Alarm will sound when seatbelt is disengaged, *Figure 13*. Resets when re-engaged, *Figure 14*.



Figure 8



Figure 9



Figure 10



Figure 11



Figure 12



Figure 13



Figure 14

WARNINGS

Before using this device with a patient, read the instructions in their entirety and familiarize yourself with the product. Ensure the seatbelt is oriented for the proper device application to prevent injury or equipment damage. Examine the device for potential damage or wear prior to use. Do not use the device if damage is visible, parts are missing, or it does not function properly. Test before each use to ensure proper operation. If seatbelt or alarm cable is damaged, discontinue use immediately.

This product is intended to be fitted and adjusted by a healthcare professional.

Care: Hand-wash, air-dry.

To Reorder

- | | | | |
|--------|--|--------|---------------------------------------|
| #79148 | Early Warning Hook-and-Loop Seatbelt | #77716 | UniLoop Attachment Sets, 3 Sets, 2/pk |
| #79147 | E-Z Release Seatbelt | #79205 | Bariatric Extender |
| #77788 | Buckled Seatbelt | | |
| #2035 | Nurse-Call Connector w/8' Cord and Y-Adapter | | |

Also available:

- #70088 Roll Control Belt w/TR2 Alarm
- #70089 Replacement Belt



MDSS GmbH
Schiffgraben 41
D-30175 Hannover,
Germany



Manufactured for:

AliMed® inc.
297 High Street
Dedham, MA 02026-9135 U.S.A.
PH 800-225-2610 • FAX 800-437-2966

AliMed.com
#6583REV0315 CCO746
©2015 AliMed® inc. All rights reserved.
Made in Taiwan

Seatbelt Adjustment and Fit

Secure seatbelt around the patient, *Figures 8 and 9*. Adjust seatbelt length by sliding buckle to shorten or increase length, *Figures 10 and 11*. If additional length is needed, a seatbelt extender (#79205) may be purchased separately.

Plug cord from seatbelt into alarm, *Figure 12*. Alarm will sound when seatbelt is disengaged, *Figure 13*. Resets when re-engaged, *Figure 14*.



Figure 8



Figure 9



Figure 10



Figure 11



Figure 12



Figure 13



Figure 14

WARNINGS

Before using this device with a patient, read the instructions in their entirety and familiarize yourself with the product. Ensure the seatbelt is oriented for the proper device application to prevent injury or equipment damage. Examine the device for potential damage or wear prior to use. Do not use the device if damage is visible, parts are missing, or it does not function properly. Test before each use to ensure proper operation. If seatbelt or alarm cable is damaged, discontinue use immediately.

This product is intended to be fitted and adjusted by a healthcare professional.

Care: Hand-wash, air-dry.

To Reorder

- | | | | |
|--------|--|--------|---------------------------------------|
| #79148 | Early Warning Hook-and-Loop Seatbelt | #77716 | UniLoop Attachment Sets, 3 Sets, 2/pk |
| #79147 | E-Z Release Seatbelt | #79205 | Bariatric Extender |
| #77788 | Buckled Seatbelt | | |
| #2035 | Nurse-Call Connector w/8' Cord and Y-Adapter | | |

Also available:

- #70088 Roll Control Belt w/TR2 Alarm
- #70089 Replacement Belt



MDSS GmbH
Schiffgraben 41
D-30175 Hannover,
Germany



Manufactured for:

AliMed® inc.
297 High Street
Dedham, MA 02026-9135 U.S.A.
PH 800-225-2610 • FAX 800-437-2966

AliMed.com
#6583REV0315 CCO746
©2015 AliMed® inc. All rights reserved.
Made in Taiwan